

# Assessing visual processing capabilities using the virtual reality device Oculus Rift

Christian H. Poth<sup>a,c</sup>, Rebecca M. Foerster<sup>a,c</sup>, Christian Behler<sup>b,c</sup>, Mario Botsch<sup>b,c</sup>, & Werner X. Schneider<sup>a,c</sup>

<sup>a</sup>Department of Psychology, Bielefeld University

<sup>b</sup>Graphics & Geometry Group, Bielefeld University

<sup>c</sup>Cluster of Excellence Cognitive Interaction Technology, Bielefeld University

c.poth@uni-bielefeld.de

## Does Oculus Rift provide sufficient test-reliability for the neuropsychological assessment of visual processing capabilities?

We assessed three visual processing components based on Bundesen's Theory of Visual Attention<sup>1,2</sup>:

- Threshold of conscious perception
- Capacity of visual working memory
- Visual processing speed



To this end, we used the virtual reality device Oculus Rift and a CRT screen, the current gold-standard.

We compared the two devices in terms of the test-retest reliability of measured visual processing components.

### Method




N = 44  
2 sessions per device, separated by 1 week

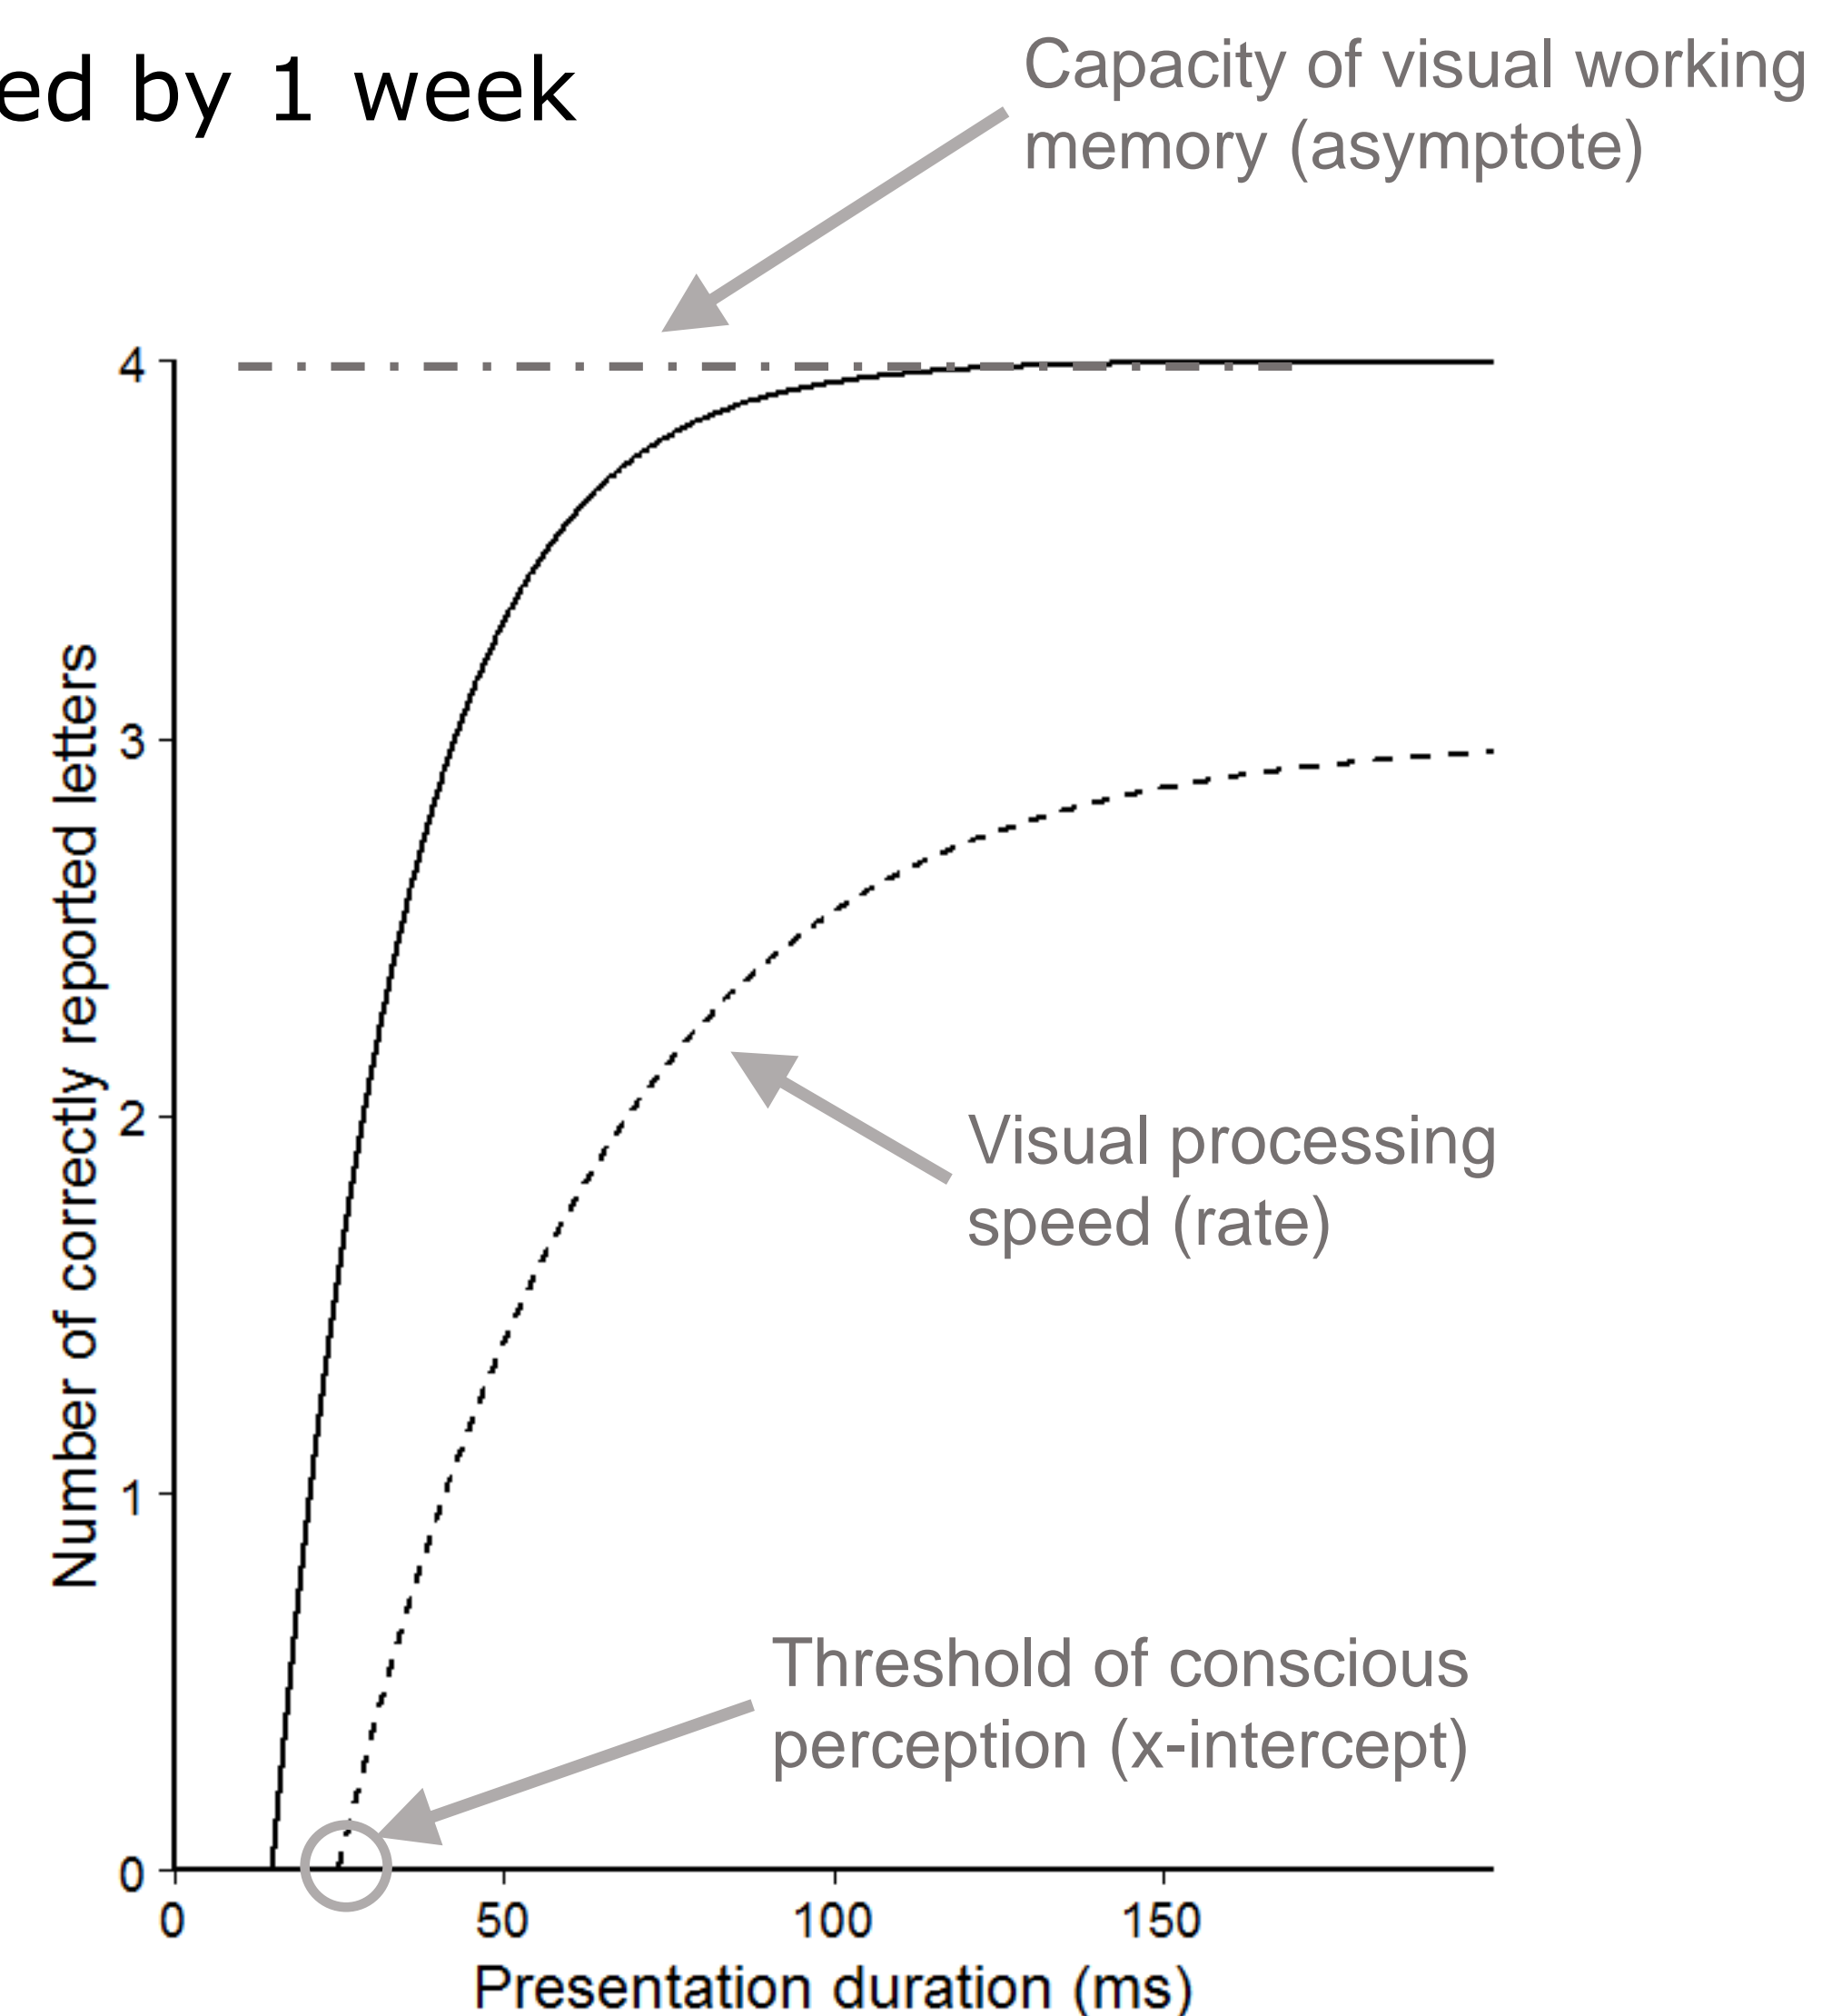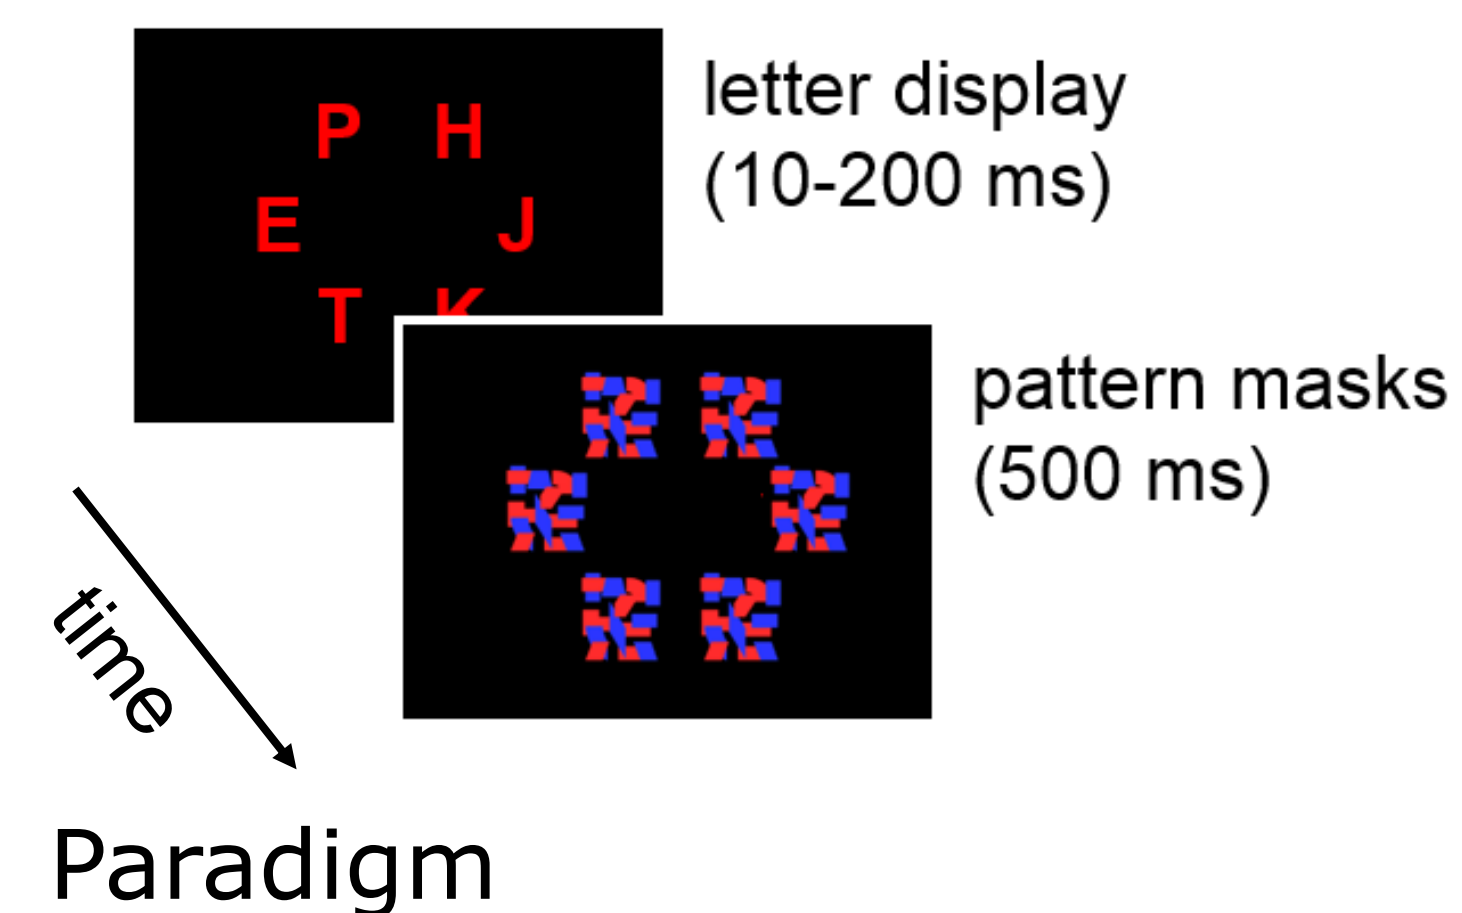

Visual processing components<sup>1,2</sup>

### Results

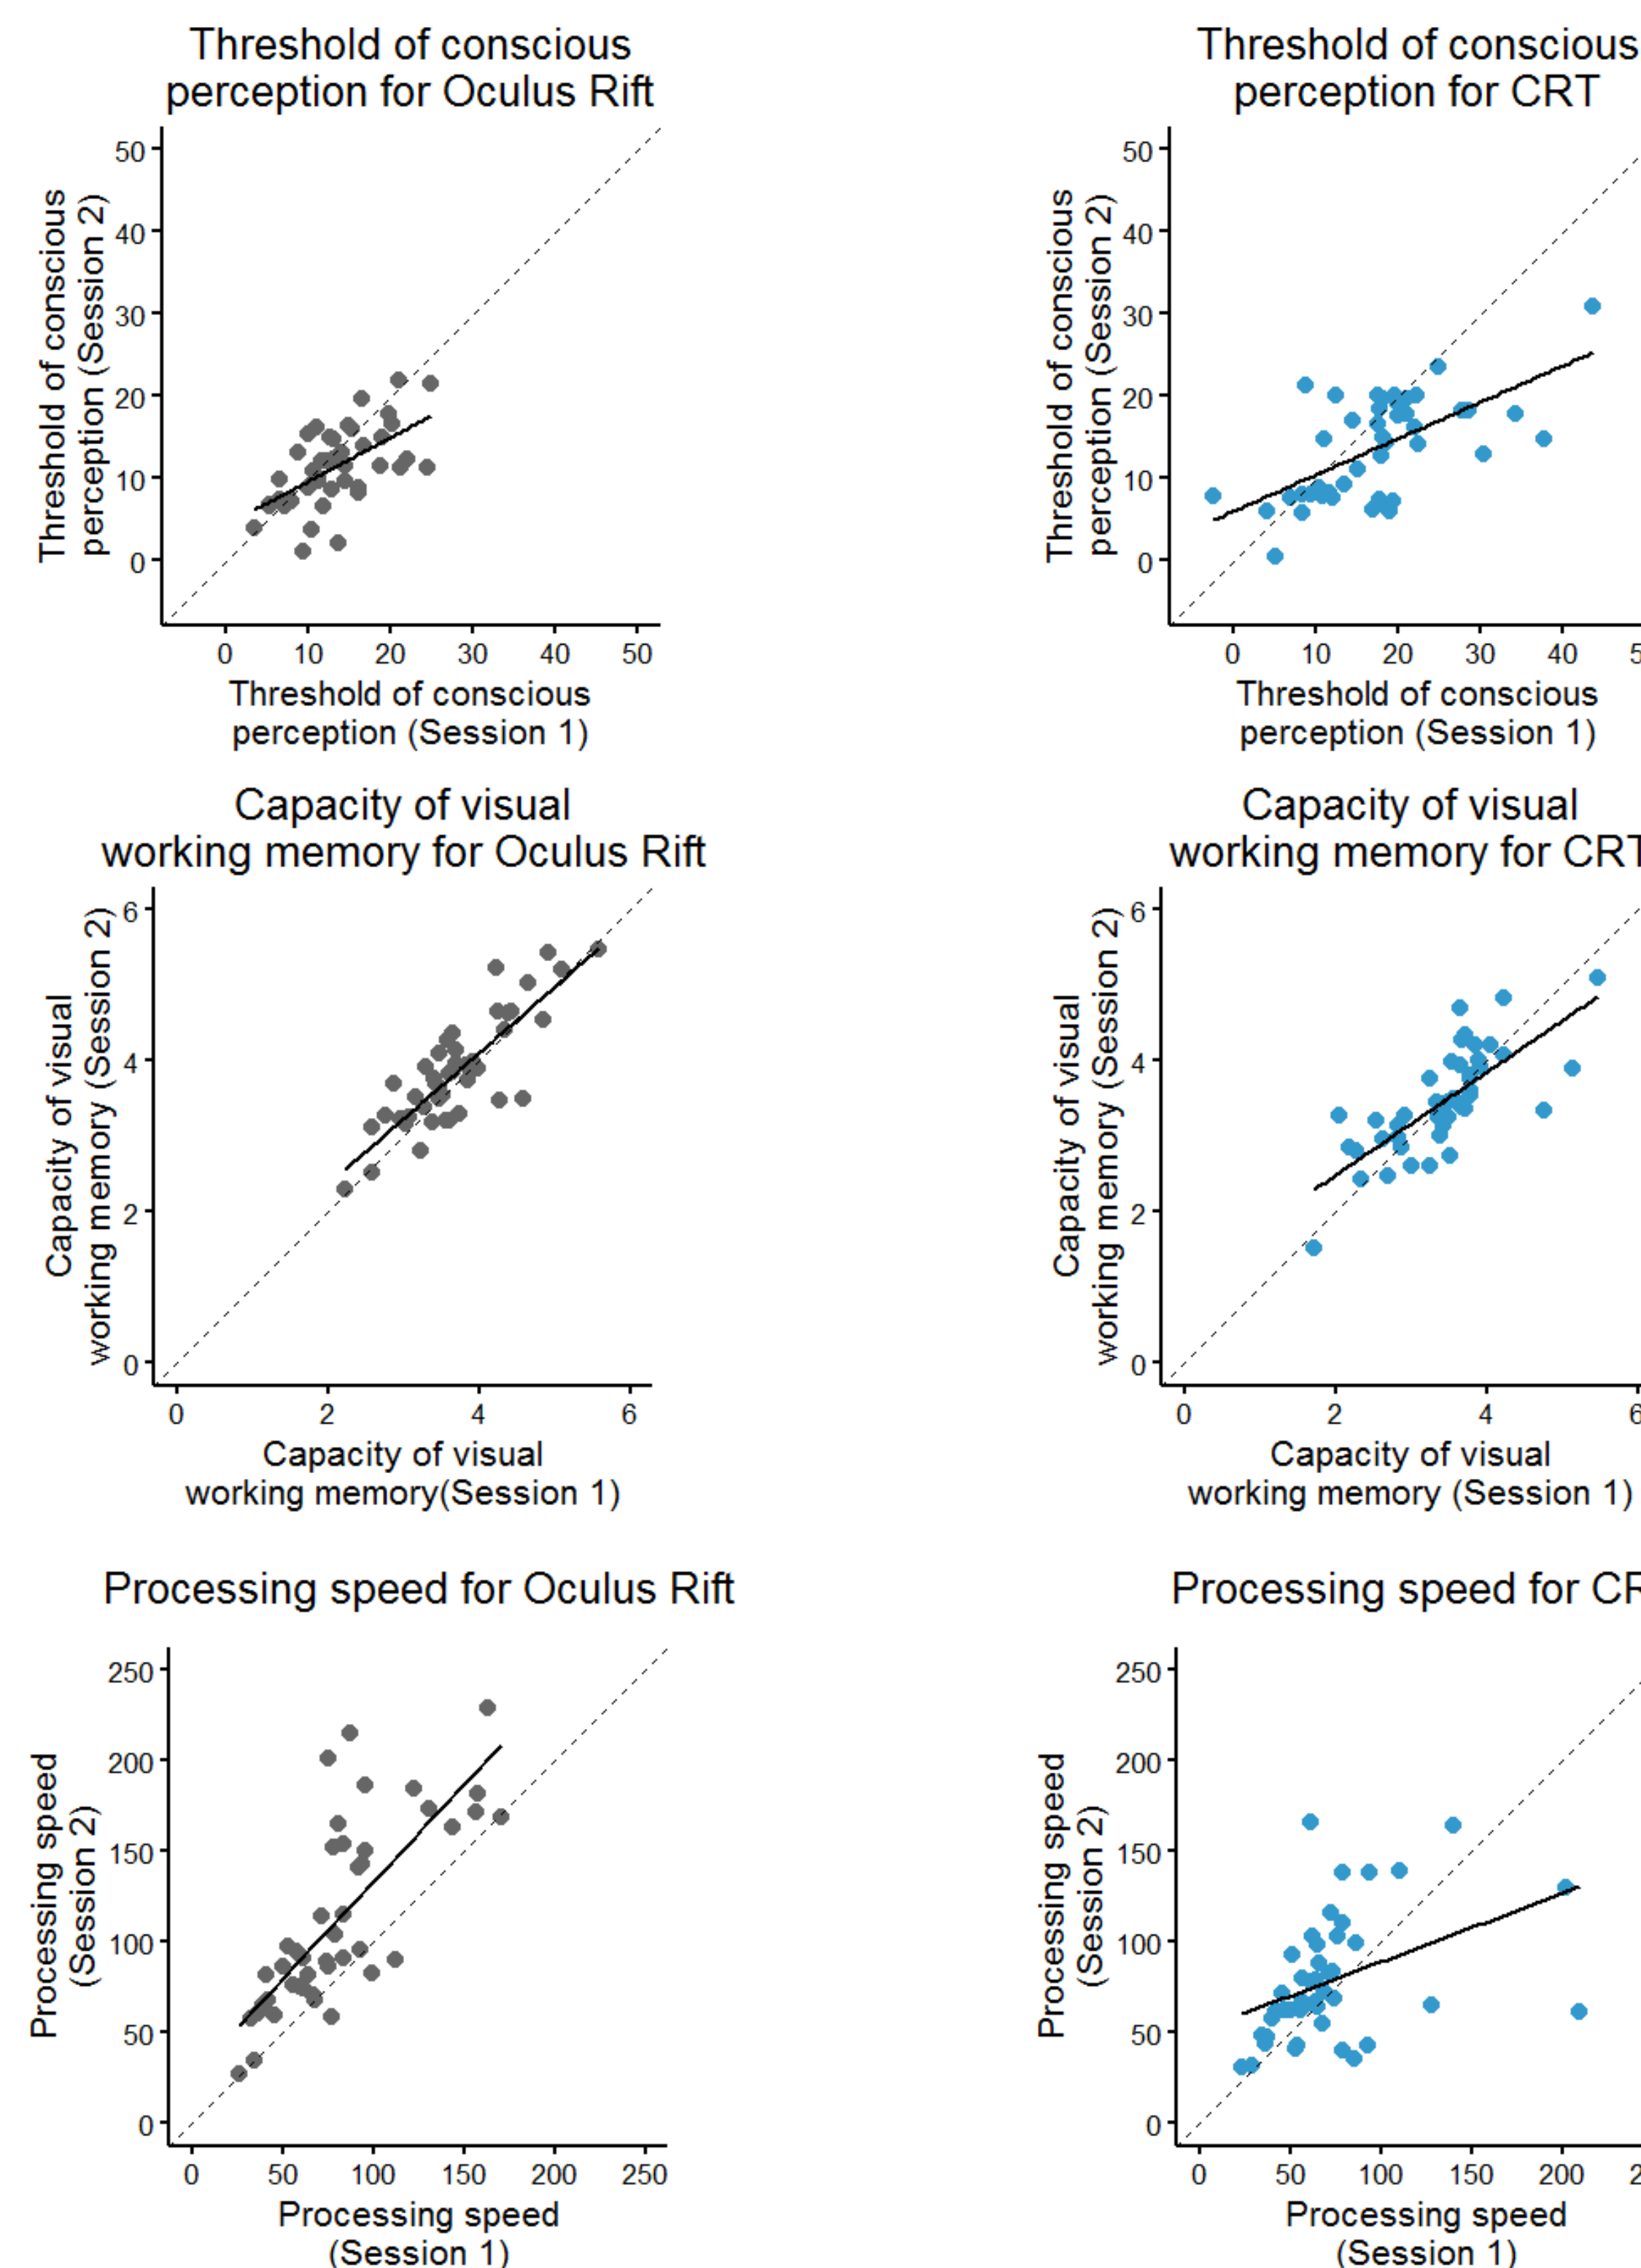

### Test-retest reliabilities (Pearson's *r*)

	Oculus Rift	CRT
	<i>r</i> ( <i>p</i> )	<i>r</i> ( <i>p</i> )
Threshold of conscious perception	.58 ( $<.001$ )	.63 ( $<.001$ )
Capacity of visual working memory	.84 ( $<.001$ )	.74 ( $<.001$ )
Processing speed	.76 ( $<.001$ )	.41 (.006)


Test-retest reliabilities did not differ between devices regarding:

- the threshold of conscious perception ( $Z = 0.391$ ,  $p = .696$ , Steiger's test)
- the capacity of visual working memory ( $Z = 1.141$ ,  $p = .254$ )

Visual processing speed was more reliably assessed with Oculus Rift than the CRT ( $Z = 2.550$ ,  $p = .011$ ).

Oculus Rift and the CRT did not differ in the test-retest reliabilities of the threshold of conscious perception and the capacity of visual working memory. For visual processing speed, Oculus Rift provided a higher test-retest reliability than the CRT.

These findings show that the virtual reality device Oculus Rift can be used for the neuropsychological assessment of visual processing capabilities.

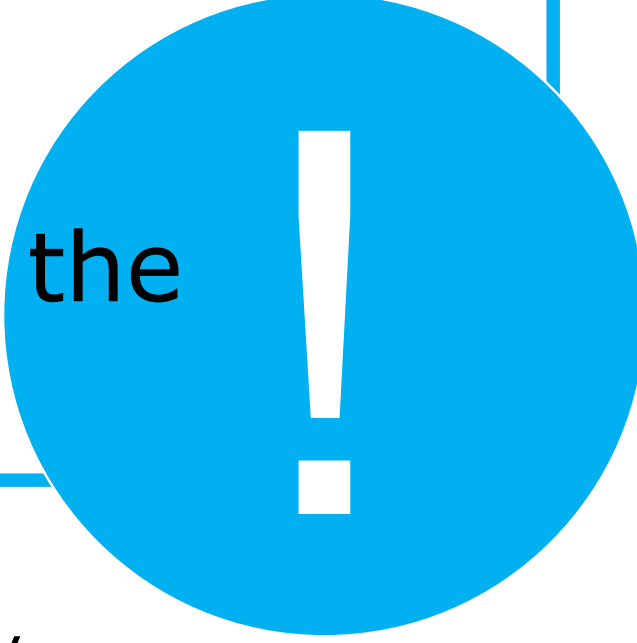

### References

- [1] Bundesen, 1990, Psych Rev
- [2] Bundesen, Vangkilde, Petersen, 2014, Vis Res